



**LilliTest Rapid NDV Ag Test Kit**  
In vitro immunochromatographic assay  
for the qualitative detection of Newcastle  
Disease Virus in avian secretions

20 x Tests/Kit



Lillidale Diagnostics  
Badbury View  
Bothenwood  
Wimborne  
Dorset  
BH21 4HU  
England

Tel: +44 (0)1202 848456  
Fax: +44 (0)1202 848570  
Email: [support@lillidale.co.uk](mailto:support@lillidale.co.uk)  
Website: [www.lillidale.co.uk](http://www.lillidale.co.uk)

Lillidale Diagnostics is a trading name of Lillidale Ltd.



# *LilliTest* Rapid NDV Ag Test Kit

For in vitro veterinary use

## Intended use

Lillitest Rapid NDV Ag Test Kit is an immunochromatographic assay for the qualitative detection of Newcastle Disease Virus Antigen (NDV Ag) in avian secretions.

## Principle

The test device has a letter of "T" and "C" as test line and control line on it's surface. Both the test line and control line in result window are not visible before applying any samples. The control line should always appear if the test procedure is performed properly and the test reagents of control line are working. A purple test line "T" will be visible in the result window if there is enough NDV antigen in the specimen. The specially selected NDV monoclonal antibodies in test band are used for both capture and detection. This enables the device to identify NDV antigen with a high degree of accuracy.

## Test kit components:

- 20 aluminium foil pouches each containing one NDV Ag card with a dropper and a desiccant
- 20 sample collection tubes containing the assay diluent
- 20 single packed swabs
- Instruction leaflet


## Sample preparation

- 1) Collect the samples from avian secretions
- 2) Insert the swab into the assay tube and gently mix until the sample dissolves in the buffer diluent.
- 3) Leave the tube until the large particles have settled to the bottom of the tube.

## Test procedure

- 1) Allow all kit components and specimen to reach room temperature prior to testing
- 2) Remove the test card from the foil pouch
- 3) Fill the pipette with the supernatant from the assay tube and drop 3 drops of the assay buffer which contains the sample into "S" well of the test card
- 4) Interpret test results at 10 minutes

## Interpretation of the results

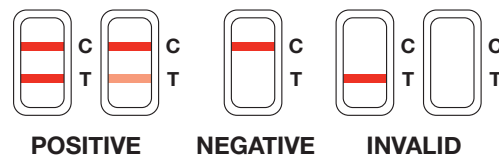

The presence of two colour bands "T" and "C" within the result window, no matter which band appears first indicates a positive result

The presence of only one band at "C" line within the result window indicates a negative result

If the control band is not visible within the result window, the result is considered invalid

## Storage Stability

The kit can be stored at room temperature (2-30°C) or refrigerated.

The test kit is stable up to the expiration date marked on the package label.

Do not freeze and do not store the test kit in direct sunlight.

## Precautions

- 1) All specimens should be handled as being potentially infectious
- 2) Do not open or remove test cards from their individually sealed pouches until immediately before their use
- 3) Do not use reagents beyond the stated expiration date marked on the package label
- 4) The components of this kit have been quality control tested as standard batch unit. Do not mix components from different lot batches

## Limitation of the test

As with all diagnostic tests the definitive diagnosis should be based on all data case history, clinical and laboratory findings etc. being evaluated by the veterinarian.

For more accuracy of immune status, additional follow-up testing using other laboratory methods is recommended.